

Replacement Sheet

7

	quantity		value
1	sphere	X	-0.30 d
	cylinder	X	-0.50 d
	axis		8°
2	pupil diameter		3.59 mm
3	analysis diameter		3.59 mm
4	Z(3, -3)		0.061 μm
	Z(3, -1)		-0.143 μm
	Z(3, 1)		-0.096 μm
	Z(3, 3)		-0.059 μm
	Z(4, -4)		0.047 μm
	Z(4, -2)		0.007 μm
	Z(4, 0)		-0.048 μm
	Z(4, 2)		-0.017 μm
	Z(4, 4)		0.002 μm
	PV OPD		2.08 μm
	RMS OPD		0.45 μm
	PV OPD HC		0.41 μm
5	RMS OPD HC		0.07 μm
	x offset		-0.53 mm
	y offset		-0.83 mm
6			

Fig. 11

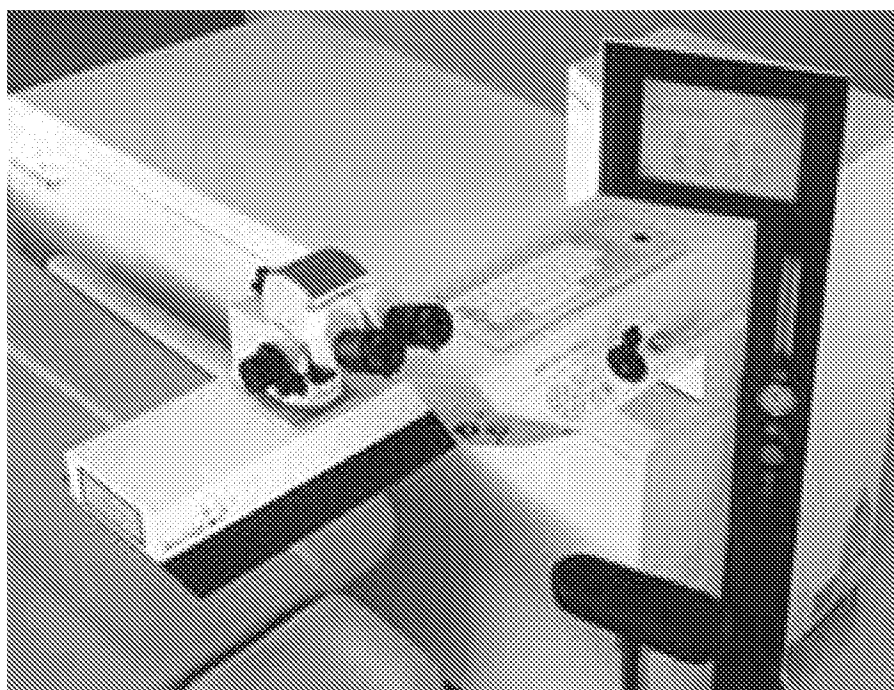


Fig. 12

Replacement Sheet

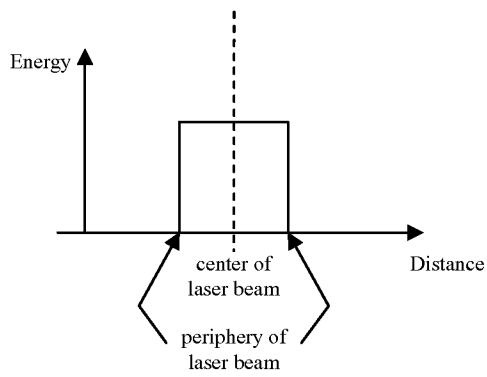


Fig. 13a

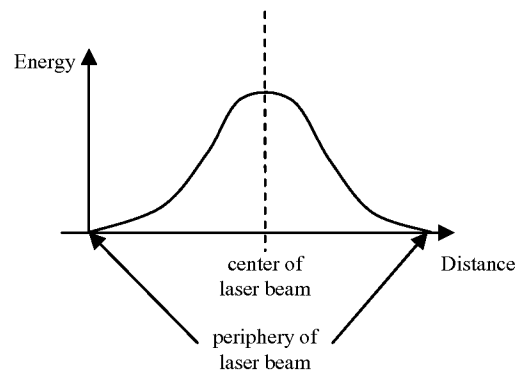


Fig. 13b

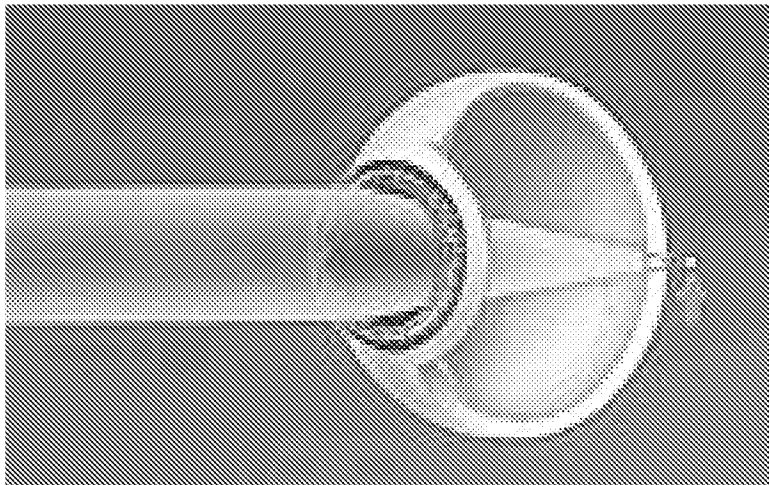


Fig. 14

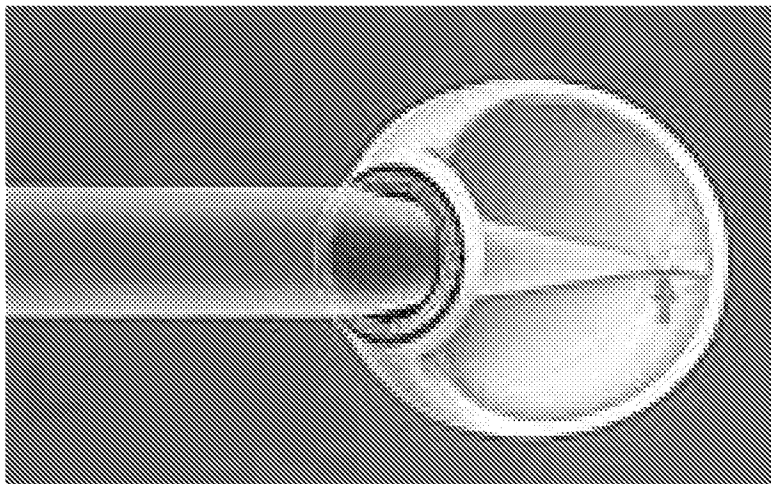


Fig. 15

Replacement Sheet

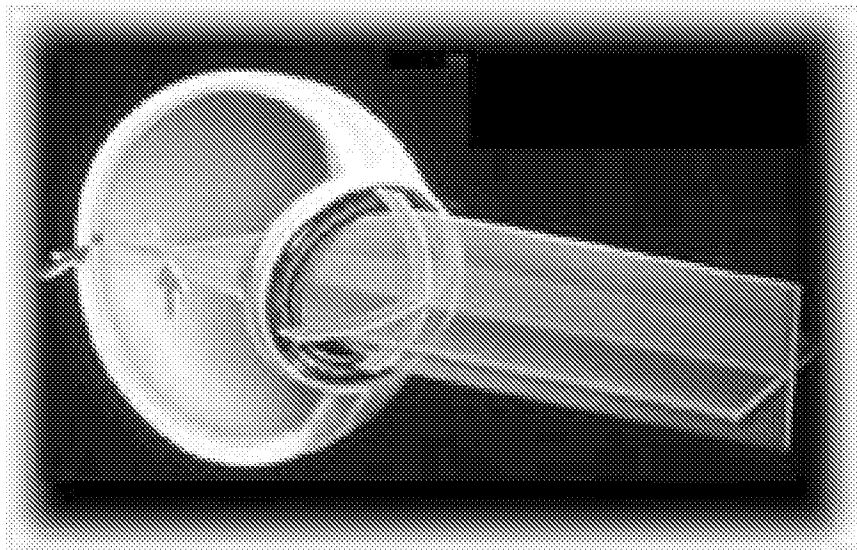


Fig. 16

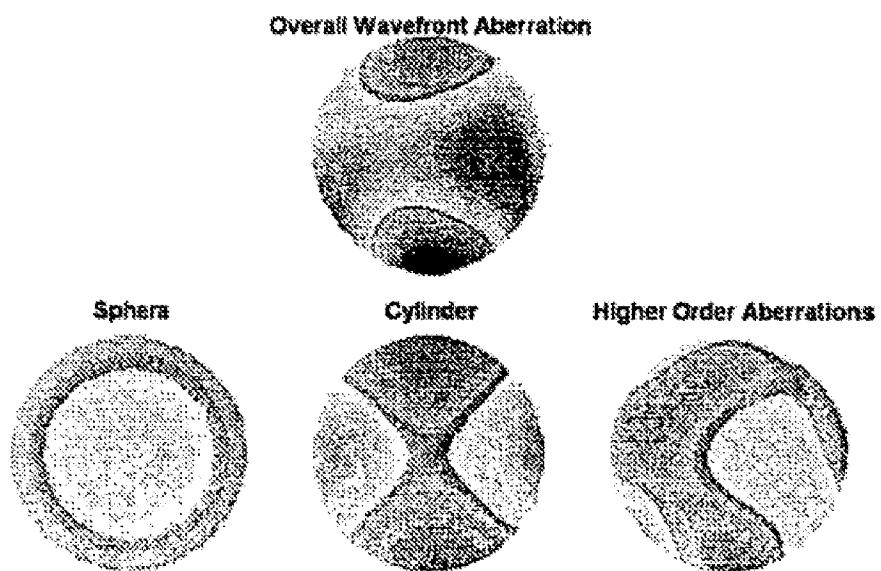


Fig. 17

Replacement Sheet

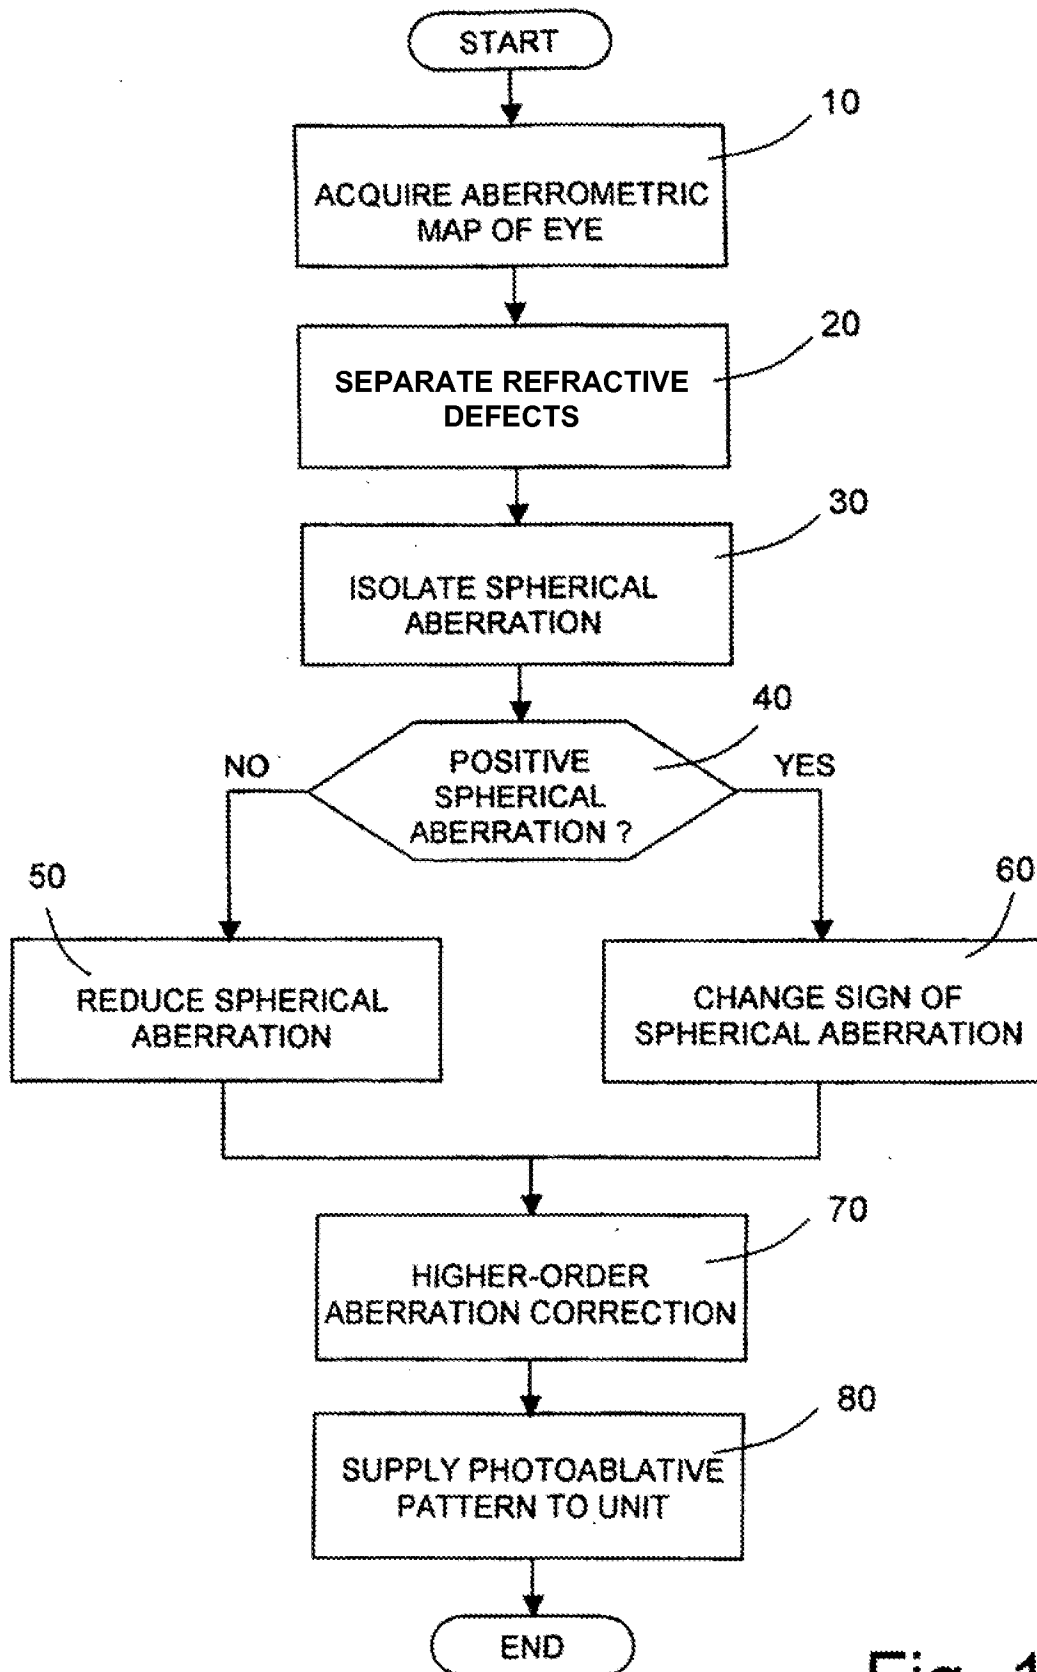


Fig. 18